OSTEOTRON IV

Ultrasound Bone Growth Stimulator

QUICK REFERENCE GUIDE




To ensure correct use, please read this guide carefully before operating the unit.


After reading, store the guide in a safe place for future reference.



- 1. Attach the probe to the strap. 🖊
- 2. Apply Ultrasound Gel to the probe and attach retainer to the treatment area.
- **3.** Press and hold the **POWER** switch (for approx. 1.5 sec) with probe connected. **/**

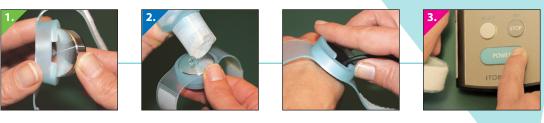

4. After the initial check is completed, the LCD screen will display the output screen, treatment will begin immediately and the timer will begin counting down.

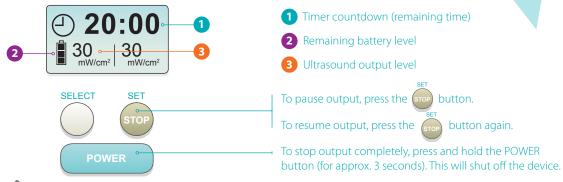

- When the remaining battery level drops to a certain level, the battery error screen will appear, and the device will shut down. If this happens, replace the batteries.
- **5.** End of treatment. When the treatment time reaches "0", the buzzer will sound and the device will shut down automatically. Remove probe from treatment area. Wipe gel from the probe. Store device in the case until the next treatment session.

Examples of output indication

